


# SALTERSTAT™ CAPNOGRAPHY

LATEX FREE | SINGLE PATIENT USE | DISPOSABLE


Designed to separate gases for accurate EtCO<sub>2</sub> signals and effective O<sub>2</sub> delivery wherever capnography is indicated. Capnography solutions for infant through adult care, .5-6 lpm O<sub>2</sub> needs, and OR and GI procedures.

## ETCO<sub>2</sub> CANNULAS

- Divided cannulas provide accurate, undiluted CO<sub>2</sub> readings—within 2-4 mm Hg of arterial CO<sub>2</sub><sup>1,2</sup>
- Also comes in SOFT headset tubing for added comfort

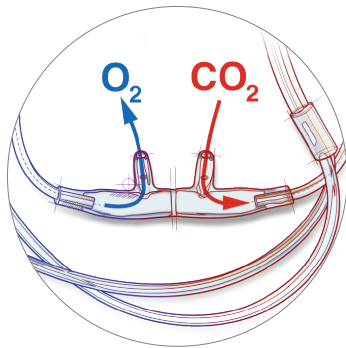


Airflow through divided cannula

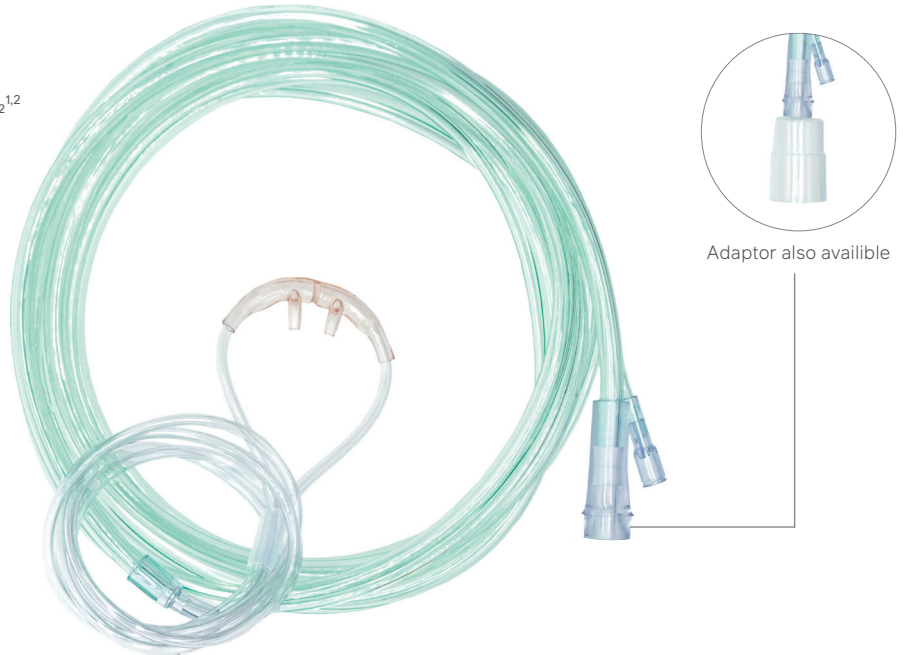

## CAPNOVUE® MASKS

Masks with CapnoVue® technology separate O<sub>2</sub> and CO<sub>2</sub> flows for procedures where higher FiO<sub>2</sub> is desired<sup>3</sup>

- Available in a variety of lengths
- Adult, pediatric, and infant sizes
- Bilateral CO<sub>2</sub> sample ports
- Offered with and without a gas sample line

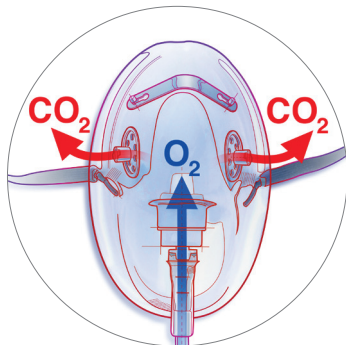

Airflow through CapnoVue mask



## DIVIDED FACEPIECES WITH SALTER EYES®

CO <sub>2</sub> /O <sub>2</sub> CONNECTOR				SIZE	O <sub>2</sub> LINE LENGTH	CO <sub>2</sub> LINE	SAMPLING LOCATION	PK
MALE/STANDARD	MALE/THREADED	FEMALE/STANDARD	FEMALE/THREADED					
4706-7-0-25	4706TG-7-0-25	4706F-7-0-25	4706FTG-7-0-25	Adult	7'	2"	Nasal	25
-	-	4796F-7-0-25	-	Adult	7'	2"	Oral/Nasal	25
4707-7-7-25	4707TG-7-7-25	4707F-7-7-25	4707FTG-7-7-25	Adult	7'	7'	Nasal	25
4797-7-7-25	4797TG-7-7-25	4797F-7-7-25	-	Adult	7'	7'	Oral/Nasal	25
4707-10-10-25	-	-	-	Adult	10'	10'	Nasal	25
4707-13-13-25	4707TG-14-14-25	-	-	Adult	13'	13'	Nasal	25
-	-	4707F-14-14-25	-	Adult	14'	14'	Nasal	25
4702-7-0-25	-	4702F-7-0-25	-	Pediatric	7'	2"	Nasal	25
4703-7-7-25	4703TG-7-7-25	4703F-7-7-25	4703FTG-7-7-25	Pediatric	7'	7'	Nasal	25
4793-7-7-25	-	4793F-7-7-25	-	Pediatric	7'	7'	Oral/Nasal	25
4701-7-0-25	-	4701F-7-0-25	-	Infant	7'	2"	Nasal	25
4700-7-7-25	-	4700F-7-7-25	4700FTG-7-7-25	Infant	7'	7'	Nasal	25
4705-7-0-25	-	4705F-7-0-25	-	Infant	7'	2"	Nasal	25
4704-7-7-25	-	4704F-7-7-25	-	Infant	7'	7'	Nasal	25

## WESTMED ETCO<sub>2</sub> SAMPLING LINES

ITEM	CONNECTORS	SUPPLY LINE	PK
0512	Male/Male	10'	50
0533	Male/Male	15'	50
0513	Male/Female	10'	50

## CAPNOGRAPHY MASK WITH CAPNOVUE TECHNOLOGY

SIZE			DESCRIPTION
ADULT	PEDIATRIC	INFANT	
4727-7-0-50	4723-7-0-50	-	Complete Mask for use with 7' Supply Line
4727TG-7-0-50	4723TG-7-0-50	4721TG-7-0-50	Complete Mask for use with 7' Supply Line and Thread Grip Connector
4727-14-0-50	-	-	Complete Mask for or use with 14' Supply Line
4727TG-14-0-50	-	-	Complete Mask for or use with 14' Supply Line and Thread Grip Connector
4737-7-0-50	4733-7-0-50	-	Scope Port for Upper-GI Procedures with 7' Supply Line
4737TG-7-0-50	4733TG-7-0-50	-	Scope Port for Upper-GI Procedures with 7' Supply Line and Thread Grip Connector
4737-14-0-50	-	-	Scope Port for Upper-GI Procedures with 14' Supply Line
4755-14-15-50	-	-	Mask, Adult with 14' O <sub>2</sub> Line And 15' CO <sub>2</sub> Sampling Line
4745-7-7-50	4745-14-15-50	-	Scope O <sub>2</sub> /CO <sub>2</sub> Mask With Luer Style Connector

\*Due to the timing of implementation across products and variable distributor inventory, a combination of soft and standard tubing divided EtCO<sub>2</sub> product will be available during the transition to soft headset tubing. Soft tubing products will state "SOFT" on the label.

References:

1. Roth JV, Barth LJ, Womack LH, Morgenlander LE. Evaluation of two commercially available carbon dioxide sampling nasal cannulae. J Clin Monit. 1994;10(4):237-243.
2. Ebert TJ, Novallija J, Uhrich TD, Barney JA. The effectiveness of oxygen delivery and reliability of carbon dioxide waveforms: a crossover comparison of 4 nasal cannulae. Anesth Analg. 2015;120(2):342-348.
3. Data on file, Salter Labs.